

4/1/99

510(k) SUMMARY

K990188

This summary of 510(k) safety and effectiveness information is submitted in accordance with the requirements of SMDA 1990 and 21 CFR 807.92.

510(k) Number: TBD

Applicant Information:

Date Prepared: January 1, 1999
Name: Intuitive Surgical, Inc.
Address: 1340 W. Middlefield Road
Mountain View, California 94043 650-237-7000
Contact Person: John N. Zorich, Jr.
Phone Number: (650) 237-7195
Facsimile Number: (650) 526-2060

Device Information:

Classification: Class II Gynecologic Laparoscope and Accessories
Rigid Endoscope
Endoscope and Accessories
Trade Name: Intuitive Surgical™ Instruments / Accessories: Endoscopic
Instruments including: Stereo Endoscope and accessories for use
with: The Intuitive Surgical™, Endoscopic Instrument Control
System
Common Name: 3D Endoscope and Accessories
Classification Name: Endoscope and Accessories 21 CFR 876.1500
Rigid Endoscope 21 CFR 876.1500
Gynecologic laparoscope and Accessories, 21 CFR 884.1720

Predicate Devices:

The Intuitive Surgical™ Endoscope is substantially equivalent in intended use and/or method of operation to the following predicate devices:

Olympus 3D Surgical Endoscopy System (Premarket Notification # K943305)
Origin/Medsystems 5mm Endoscope (Premarket Notification # K960637)

003

510(k) SUMMARY (Continued)

Device Description:

The Intuitive Surgical™ Stereo View System consists of an Intuitive Surgical endoscope, an Intuitive Surgical camera, and a commercially available light source. The endoscope is essentially identical in size and shape to the predicate devices referenced above, with minor modifications so that it can be attached to the Intuitive Surgical™ Endoscopic Instrument Control System. The camera and illumination sources attach to the endoscope and are essentially identical in function to those incorporated with the predicate Olympus System.

Intended Use:

The Intuitive Surgical™ Stereo View Endoscopic System is intended for endoscopic viewing of internal surgical sites during minimally invasive surgery in the peritoneal cavity, thoracic cavity, and peritoneum. It is designed to be used with the Intuitive Surgical™ Endoscopic Instrument Control System during thoracoscopic and laparoscopic surgical procedures.

Comparison to Predicate Devices:

The Intuitive Surgical™ Stereo View Endoscopic System endoscopes are essentially identical in terms of shape, size, materials, and function to the standard endoscopes cited. The stereo view feature of the camera is essentially identical to the 3D feature of the predicate Olympus System. The illumination source is identical to the one in the predicate Olympus system.

Test Data:

Design analysis and comparison confirm that basic functional characteristics are substantially equivalent to the predicate devices cited.

Summary:

Based upon the product technical information provided, intended use, and performance information provided in this pre-market notification, the Intuitive Surgical Stereo View Endoscopic System has been shown to be substantially equivalent to currently marketed predicate devices.

Intuitive™ and Intuitive Surgical™ is a registered trademark of Intuitive Surgical, Inc.



Food and Drug Administration
9200 Corporate Boulevard
Rockville MD 20850

APR 1 1999

Mr. John N. Zorich, Jr.
Manager, Quality Systems and Regulatory Compliance
Intuitive Surgical, Inc.
1340 West Middlefield Road
Mountain View, California 94043

Re: K990188
Trade Name: Intuitive Surgical™ Stereo View Endoscopic System
Regulatory Class: II
Product Code: GCJ
Dated: January 19, 1999
Received: January 20, 1999

Dear Mr. Zorich:

We have reviewed your Section 510(k) notification of intent to market the device referenced above and we have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.


If your device is classified (see above) into either class II (Special Controls) or class III (Pre-market Approval), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 895. A substantially equivalent determination assumes compliance with the current Good Manufacturing Practice requirement, as set forth in the Quality System Regulation (QS) for Medical Devices: General regulation (21 CFR Part 820) and that, through periodic (QS) inspections, the Food and Drug Administration (FDA) will verify such assumptions. Failure to comply with the GMP regulation may result in regulatory action. In addition, FDA may publish further announcements concerning your device in the Federal Register. Please note: this response to your premarket notification submission does not affect any obligation you might have under sections 531 through 542 of the Act for devices under the Electronic Product Radiation Control provisions, or other Federal laws or regulations.

Page 2 – Mr. John N. Zorich, Jr.

This letter will allow you to begin marketing your device as described in your 510(k) premarket notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801 and additionally 809.10 for in vitro diagnostic devices), please contact the Office of Compliance at (301) 594-4595. Additionally, for questions on the promotion and advertising of your device, please contact the Office of Compliance at (301) 594-4639. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR 807.97). Other general information on your responsibilities under the Act may be obtained from the Division of Small Manufacturers Assistance at its toll-free number (800) 638-2041 or (301) 443-6597 or at its internet address "<http://www.fda.gov/cdrh/dsmamain.html>".

Sincerely yours,

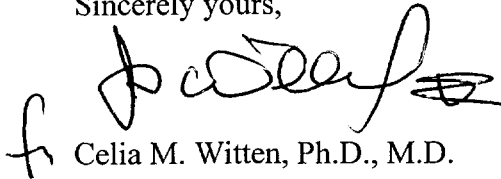A handwritten signature in black ink, appearing to read 'C. Witten', with a stylized flourish at the end.

Celia M. Witten, Ph.D., M.D.
Director
Division of General and
Restorative Devices
Office of Device Evaluation
Center for Devices and
Radiological Health

Enclosure

510(k) Number (if known): TBD K990188


Device Name: Intuitive Surgical™ Stereo View Endoscopic System

Indications For Use:

The Intuitive Surgical™ Stereo View Endoscopic System is intended for endoscopic viewing of internal surgical sites during minimally invasive surgery in the peritoneal cavity, thoracic cavity, and peritoneum. It is designed to be used with the Intuitive Surgical™ Endoscopic Instrument Control System during thoracoscopic and laparoscopic surgical procedures

(PLEASE DO NOT WRITE BELOW THIS LINE - CONTINUE ON ANOTHER PAGE IF NEEDED)

Concurrence of CDRH, Office of Device Evaluation (ODE)

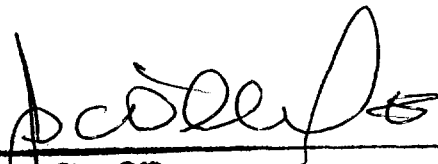

(Division Sign-Off)
Division of General Restorative Devices K990188
510(k) Number _____

Prescription Use X
(Per 21 CFR 801.109)

OR

Over-The-Counter Use _____

(Optional Format 1-2-96)

Page 9